

Effect of Fabrication Method and Heat Treatment on the Properties of Co-Cr Bio Alloy

Zahraa A. Hanoon ^{1,*}, Adnan S. Jabur ²

¹ Department of Mechanical Engineering, College of Engineering, University of Basrah, Basrah, Iraq

² Department of Material Engineering, College of Engineering, University of Basrah, Basrah, Iraq

E-mail addresses: zahraaayadhanon@gmail.com, adnan.jabur@uobasrah.edu.iq

Received: 24 November 2022; Revised: 22 January 2023; Accepted: 31 January 2023; Published: 30 December 2023

Abstract

Co-Cr alloys are widely used in dental and medical equipment since the development of the first cast Co-Cr-Mo alloy. This is due to its high mechanical properties and high resistance to wear and corrosion. This research aims to study the effect of the fabrication method (Investment Casting and Selective Laser Melting SLM by 3D printing) and heat treatments on the mechanical and tribological properties of Co-Cr-Mo alloy. It was found that the Selective Laser Melting method in general increases the ultimate tensile strength, strain and hardness compared to the Investment Casting method. Also, solution treatment and aging reduce the strength and strain values of the SLM samples and have no obvious effect on the casting samples. The wear test shows that wear rate of casting samples is lower than that of SLM samples.

Keywords: Co-Cr-Mo alloy, Investment casting, Selective laser melting, hardness, wear, ultimate strength.

© 2023 The Authors. Published by the University of Basrah. Open-access article.

<https://doi.org/10.33971/bjes.23.2.6>

1. Introduction

Co-Cr alloys have been discovered since the beginning of 1900s and the Stellite alloys manufactured by Haynes became important materials for wear-resistant applications [1]. Due to their exceptional mechanical, wear and corrosion properties, Co-Cr alloys are considered as effective biomaterials and have been used in applications of medical and dental parts. Since the development of the cast Co-Cr-Mo alloy in the 1930s and the use of the lost-wax method in its manufacture, its commercial use has become widespread [2-3]. The lost wax method suffers from the problem that it is sensitive to human error [4].

Recently, advanced manufacturing methods using computer-aided design / computer-aided manufacturing (CAD/CAM) for the production of biomedical devices and dental prostheses have been established [5-7].

A CAD/CAM technology-based Additive manufacturing is an excellent alternative to the traditional Investment wax casting method in producing restorations. One of the additive manufacturing methods is selective laser melting (SLM), in which parts can be made directly from a three-dimensional CAD model by fusing metal powder and building layers using a focused laser beam [8]. Also, many researchers have found that SLM-manufactured parts have higher mechanical properties than those manufactured by the casting method [4].

Figure 1 includes the equilibrium phase diagram for the Co-Cr system. It shows that pure cobalt undergoes martensitic change at 417° C from γ -phase (FCC) to ϵ -phase (HCP) [10-11].

The transformation temperature is changed by the addition of alloying elements to Co., So it changes to 900° C for Co-Cr alloys.

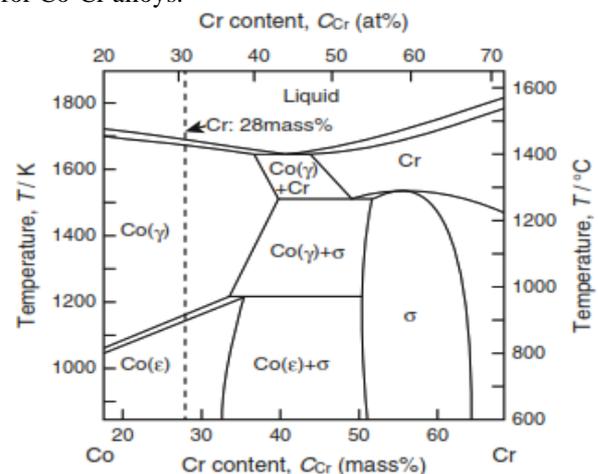


Fig.1 Equilibrium phase diagram of Co-Cr alloys [9]

Co-Cr alloys manufactured with conventional casting have a dendritic structure. The dendritic and interdendritic regions are of γ -phase and ϵ -phase respectively. Although the phase diagram specifies that there is only a ϵ -phase at room temperature, in fact there is a residual γ -phase due to the slow γ - ϵ transition. [12]. X-ray diffractometry shows that the amount of ϵ -phase increases significantly from 2% for the Laser surface processing to 13% in the as cast specimen, 24% in the annealed specimen, and 51% for the TIG surface processing [13].

On the other hand, the structure of Co-Cr alloys produced by SLM is homogeneous comprised of fine cellular dendrites [14]. The average hardness was higher than that of other fabrication processes. Some investigators have studied Co-Cr-Mo alloy devices manufactured by direct laser sintering. They found that the microstructure consists of γ and ϵ phases. Whereas, ϵ phase consists of a network of thin layers within γ phase. They explained the high hardness of the alloy as being due to the obstruction of the ϵ phase layers to the movement of dislocations in the γ phase [15].

The γ -phase is ductile, while the ϵ -phase is hard, so increases wear and corrosion resistance [16]. Therefore, the properties of Co-Cr alloys depend on the ratio of γ to ϵ as well as the percentage of carbides present [17].

Heat treatments are usually used to relieve stresses and improve the mechanical properties of traditional casting parts [18-20]. AM parts also employ heat treatment for reduction of internal stresses but improvement in their elongation and the fatigue performance is also possible [21]. Its conditions affect the size, shape, and distribution of precipitates [22-24], size and shape of grains [25-27], and γ/ϵ fraction [24-28].

The following heat treatment for the investment cast alloy includes the solution treatment at a temperature of 1200 to 1255 °C for a period of 1-3 hours, followed by cooling with water and then aging at a temperature of 800 to 900 °C [29]. The objective of this heat treatment is to homogenize the cast structure, eliminate segregation, enhance martensitic change, and deposit fine carbides [30]. As for the SLM, its resulting microstructure differs greatly from the investment as cast structure, and therefore it needs a different heat treatment to improve its properties. SLM involves local melting of small areas of metal powder, which solidifies at a very high out-of-equilibrium speed, which results in a very fine supersaturated microstructure of products [31-32]. Therefore, the heat treatment should take those structural characteristics in consideration and avoid the growth of the fine microstructure.

The aim of this research is to study the effect of fabrication method and heat treatments on the mechanical properties of Co-Cr alloys.

2. Experimental Procedure

2.1 Samples Preparation

Two sets of samples were prepared for each of the investment and SLM processes. Each including three individual samples (see Fig. 2). These samples belong to the class of mediloy® S-Co of standards; ISO 22674 and ISO 9693. The chemical composition of this alloy is in table 1.



Fig.2 a) Investment casting sample (10X4X65 mm) b) Selective Laser Melting sample (10X4X80 mm)

Co	Cr	Mo	W	Si
63.9	24.7	5	5.4	1

2.2 Processing Conditions

Table 2 includes the various conditions of the processes conducted on the samples for this research.

Table 2 Samples conditions

Sample code	conditions
La	SLM as prepared samples
Lhs	SLM + Solution treated at 1100°C for 3 hrs.
Lha	SLM + Solution treated at 1100°C for 3 hrs. + Aged at 800°C for 2 hrs.
Ca	Investment As Cast samples
Chs	Inv. Casting + Solution treated at 1100°C for 3 hrs.
Cha	Inv. Casting + Solution treated at 1100°C for 3 hrs. + Aged at 800°C for 2 hrs.

2.3 Study Testing

Three types of tests were performed on all samples under the conditions mentioned in table 2. These tests include tensile, hardness and wear testing. Each test was repeated three times on three samples from the same conditions, and the average of the test results was taken for them. The tensile test was carried out with a universal tensile device. The tensile samples were prepared in accordance with ASTM Standard (E8-91) [33]. (Fig.3) shows two tensile samples after testing. The hardness test was performed by the Vickers hardness device. The wear test was carried out with a pin-on-ring device (Fig.4). Diameter of the ring was 4.6 cm. The wear rate was measured by measuring the weight lost during rubbing divided by the rubbing distance.

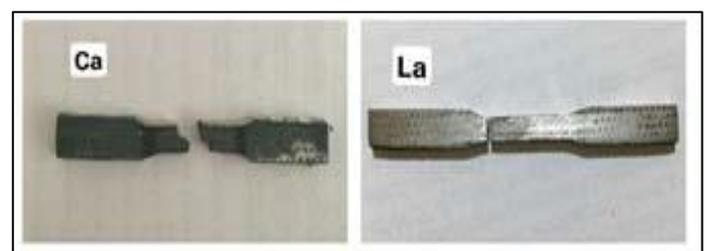


Fig.3 Two types of Tensile samples after Testing



Fig. 4 Pin on Ring device of Wear Testing

3. Results and Discussion

3.1 Tensile Test

Figures 5 and 6 show the tensile strength and Max. strain bar charts of the SLM and Investment casting samples in different conditions respectively. They show that the ultimate tensile strength and strain values of the samples manufactured by SLM are much higher than that of the samples manufactured by the investment casting. This can be explained by the fact that the samples manufactured with SLM have a fine dendritic and homogenous structure compared to those manufactured with casting [14]. They also show that the solution treatment and aging of the SLM-manufactured samples cause a decrease in the ultimate tensile strength and strain values, but they do not have a clear effect on the samples manufactured by investment casting. This is because these heat treatments lead to the growth of grains and a decrease in the strength and strain.

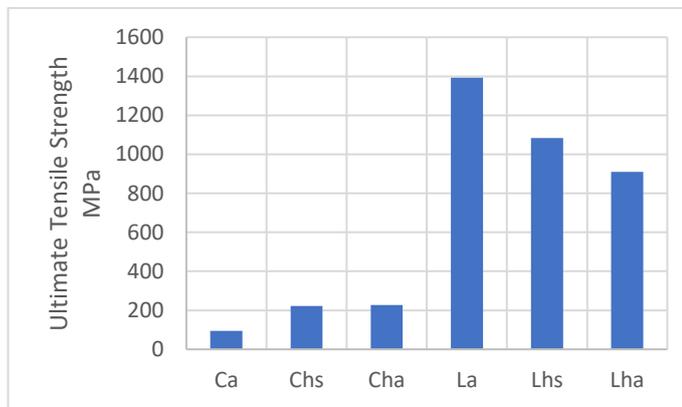


Fig.5 Ultimate tensile strength value of samples

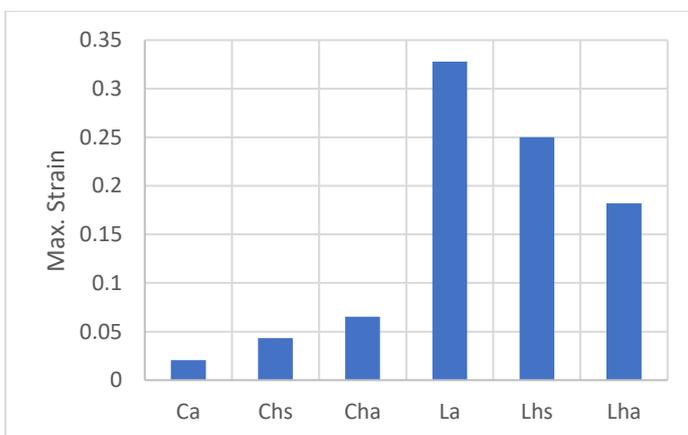


Fig. 6 Maximum strain value of samples

3.2 Hardness Test

Figure 7 includes a bar chart for the Vickers hardness values for all conditions of manufacturing and heat treatments. It shows that the samples manufactured with SLM have a higher hardness than those manufactured with casting. This is due to the same reason mentioned in the previous paragraph, which is the fine dendritic structure resulting from the high freezing rate in the SLM method compared to the slow rate of freezing in the casting method. The figure also shows that there is no significant effect of heat treatments on the hardness values of the two manufacturing methods.

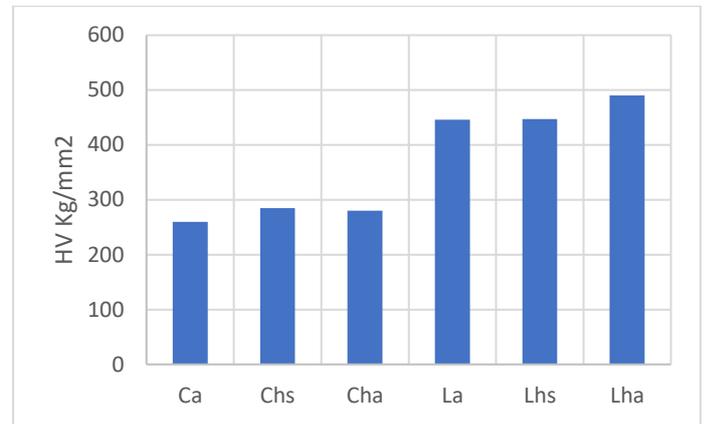


Fig.7 Vickers Hardness values of samples

3.3 Wear Test

Figure 8 includes the wear rate values for all conditions of manufacturing and heat treatments. The figure shows that the wear rate resulting from the weight loss of the cast-manufactured samples is generally lower than that of the SLM-manufactured samples. This is illogical if we take the hardness values of these samples (Fig.7) into consideration. Because it is known that the wear rate of the metal decreases with increasing hardness. This can be explained by the fact that the cast samples are so soft that there will be plastic deformation of the rubbing surfaces instead of removing the metal. Therefore, wear rate values for cast samples cannot be reliable.

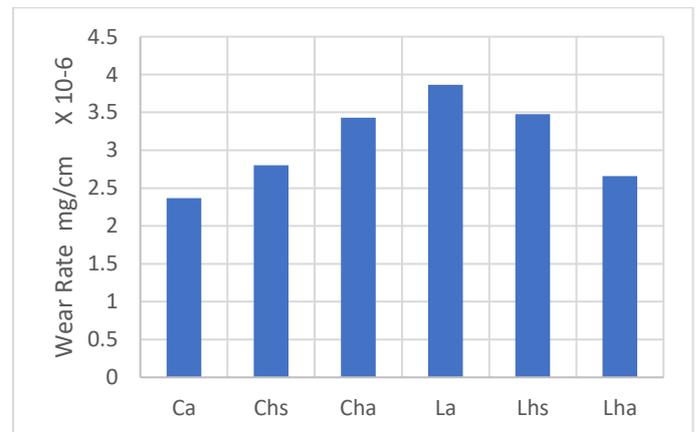


Fig. 8 Wear rate value of samples

4. Conclusions

- 1- Samples manufactured by SLM method have much higher tensile strength and strain than samples manufactured by the traditional method of investment casting.
- 2- Heat treatments such as solution treatment and aging caused a decrease in the tensile stress and strain values of the SLM-fabricated samples, but they had no significant effect on the cast-fabricated samples.
- 3- The samples manufactured with SLM have a higher hardness than those manufactured with investment

casting, but heat treatments have no significant effect on the hardness values of the two manufacturing methods.

- 4- The wear rate of the cast-fabricated samples is generally lower than that of the SLM-fabricated samples.

References

- [1] Takayuki Narushima, Kyosuke Ueda Tohoku University, Alfirano Alfirano UNTIRTA. "Co-Cr Alloys as Effective Metallic Biomaterials" January 2015.
[DOI: 10.1007/978-3-662-46836-4_7](https://doi.org/10.1007/978-3-662-46836-4_7).
- [2] Morral FR, "Cobalt alloys as implants in humans". *J Mater* (1966), Vol. 1 pp:384–412.
- [3] Morral FR, "The metallurgy of cobalt alloys – a 1968 review", (1968), *J Met* Vol. 20, pp:52–59.
- [4] Eggbeer D., Ribb R., Williams R. "The computer-aided design and rapid prototyping fabrication of removable partial Mechanical Engineers. Part H: *Journal of Engineering in Medicine*, (2005), 219/3, pp195–202.
<https://doi.org/10.1243/095441105X9372>
- [5] Ucar, Y.; Brantley, W.A.; Johnston, W.M.; Dasgupta, T. "Mechanical properties, fracture surface characterization, and microstructural analysis of six noble dental casting alloys". *J. Prosthet. Dent.* (2011), vol. 105, pp: 394–402.
- [6] Hedberg, Y.S.; Qian, B.; Shen, Z.; Virtanen, S.; Wallinder, I.O. "In vitro biocompatibility of CoCrMo dental alloys fabricated by selective laser melting". *Dent. Mater.* (2014), vol.30, pp. 525–534.
- [7] Jang, S.H.; Lee, D.H.; Ha, J.Y.; Hanawa, T.; Kim, K.H.; Kwon, T.Y. "Preliminary evaluation of mechanical properties of Co-Cr alloys fabricated by three new manufacturing processes". *Int. J. Prosthodont.* (2015), Vol. 28, pp. 396–398
- [8] Koutsoukis, T.; Zinelis, S.; Eliades, G.; Al-Wazzan, K.; Rifaiy, M.A.; Al Jabbari, Y.S. "Selective laser melting technique of Co-Cr dental alloys: A review of structure and properties and comparative analysis with other available techniques. *J. Prosthodont.* (2015), vol. 24, pp:303–312.
- [9] Baker H (ed), *ASM handbook, "Alloy phase diagrams"*. ASM International, Materials Park, (1992), vol.3 pp: 2–140.
- [10] Davis JR (ed). *ASM specialty handbook, "nickel, cobalt, and their alloys"*. ASM International, Materials Park, (2000), pp:356.
- [11] Beltran AM "Cobalt-base alloys". In: Sims CT, Stoloff NS, Hagel WC (eds) *Superalloys II*. Wiley, New York, (1987), pp:135–163.
- [12] Lopez HF, Saldivar-Garcia AJ. "Martensitic transformation in cast Co–Cr–Mo–C alloy". *Metall Mater Trans A*, (2007), vol.39, pp: 8–18.
- [13] Vladimir Vega Valer. "Thermal Cooling Effects in the Microstructure and Properties of Cast Cobalt-Base Biomedical Alloys". *Theses and Dissertations for University of Wisconsin-Milwaukee*, August (2014).
<https://dc.uwm.edu/etd/844>
- [14] Meacock C.G., Vilar R. "Structure and properties of a biomedical Co–Cr–Mo alloy produced by laser powder microdeposition". *Journal of Laser Applications*, (2009), vol.21, pp:88 – 95.
- [15] Barucca G., Santecchia E., Majni G. "Structural characterization of biomedical Co-Cr-Mo components produced by direct metal laser sintering". *Science and Engineering C*, (2015), vol.48, pp: 263 – 269.
- [16] Torabi K., Farjood E., Hamedani Sh. "Rapid prototyping technologies and their applications in prosthodontics, a Review of Literature". *Journal of Dentistry (Shiraz Univ. Med. Sci.)*, 16 (1), (2015), pp. 1 – 9.
- [17] N.A. Dolgov1a, Ts. Dikova2b, Dzh. Dzhendov2c, D. Pavlova3d, M. Simov3e. "Mechanical properties of dental Co-Cr alloys fabricated via casting and selective laser melting". *Scientific proceedings international scientific-technical conference "innovations in engineering"*, (2016), ISSN 1310-3946.
- [18] Mohammed Jacob Joseph and Murtadha Abbas Jabbar. "Effect of aging process on the microstructure, corrosion resistance and mechanical properties of stainless steel AISI 204." University of Basra-College of Engineering, Mechanical Engineering Department, Iraq, 2019.
<https://doi.org/10.1016/j.cscem.2019.e00253>
- [19] Haider M Mohammad, Haider Mahdi Lieth, Murtadha Abbas Jabbar. "Estimation of residual stresses in quenched 4140 low alloy steel using x-ray diffraction (xrd)." Department of Materials Engineering, College of Engineering, University of Basrah, 2022.
[DOI : 10.35741/issn.0258-2724.57.3.31](https://doi.org/10.35741/issn.0258-2724.57.3.31)
- [20] Brantley, W.A. and Alapati. "Heat Treatment of Dental Alloys", (2012), A Review available at
<http://dx.doi.org/10.5772/52398>
- [21] Thöne, M., Leuders, M., Riemer, A., Tröster, T and Richard. "Influence of heat-treatment on Selective Laser Melting products – e.g. Ti6Al4V", (2012), available at
<http://utwired.engr.utexas.edu/lff/symposium/proceedingsArchive/pubs/Manus>
- [22] Mengucci, P., Barucca, G., Gatto, A., Bassoli, E., Denti, L., Fiori, F., Girardin, E., Bastianoni, P., Rutkowski, B., Czyska-Filemonowicz, A., 2016. Effects of thermal treatments on microstructure and mechanical properties of a Co-Cr-Mo-W biomedical alloy produced by laser sintering. *J Mech Behav Biomed Mater* Vol. 60, pp: 106-117.
- [23] Takaichi, A., Suyalatu, Nakamoto, T., Joko, N., Nomura, N., Tsutsumi, Y., Migita, S., Doi, H., Kurosu, S., Chiba, A., Wakabayashi, N., Igarashi, Y., Hanawa, T., 2013. Microstructures and mechanical properties of Co-29Cr-6Mo alloy fabricated by selective laser melting process for dental applications. *J Mech Behav Biomed Mater* Vol.21, pp:67 -76.
- [24] Wei, W., Zhou, Y., Sun, Q., Li, N., Yan, J., Li, H., Liu, W., Huang, C., 2020. Microstructures and Mechanical Properties of Dental Co-Cr-Mo-W Alloys Fabricated by Selective Laser Melting at Different Subsequent Heat Treatment Temperatures. *Metallurgical and Materials Transactions A* Vol.51, pp:3205-3214.
- [25] Kittikundecha, N., Kajima, Y., Takaichi, A., Wai Cho, H.H., Htat, H.L., Doi, H., Takahashi, H., Hanawa, T., Wakabayashi, N., 2019. Fatigue properties of removable partial denture clasps fabricated by selective laser melting followed by heat treatment. *J Mech Behav Biomed Mater*, Vol.98, pp:79-89.
- [26] Seki, E., Kajima, Y., Takaichi, A., Kittikundecha, N., Cho, H.H.W., Htat, H.L., Doi, H., Hanawa, T., Wakabayashi, N., 2019. Effect of heat treatment on the microstructure and fatigue strength of CoCrMo alloys fabricated by selective laser melting. *Materials Letters*, Vol.245, pp: 53-56.
- [27] Takaichi, A., Kajima, Y., Kittikundecha, N., Htat, H.L., Wai Cho, H.H., Hanawa, T., Yoneyama, T., Wakabayashi, N., 2020. Effect of heat treatment on the anisotropic microstructural and mechanical properties of Co-Cr-Mo alloys

produced by selective laser melting. *J Mech Behav Biomed Mater* 102, 103496.

[28] Zhou, Y., Sun, Q., Dong, X., Li, N., Shen, Z.J., Zhong, Y., Eriksson, M., Yan, J., Xu, S., Xin, C., 2020. Microstructure evolution and mechanical properties improvement of selective laser melted Co-Cr biomedical alloys during subsequent heat treatments. *Journal of Alloys and Compounds*, Vol.840, pp:155664.

[29] R. Narayan, *ASM Handbook, "Materials for Medical Devices"*. ASM International, (2012), Vol.32.

[30]R. Pillar, S.D. Ramsay." Cobalt-base alloys". in: R.J. Narayan (Ed.), *Mater. Med. Devices*, ASM International, (2012),pp: 211–222.

doi:10.31399/asm.hb.v23.a0005669.

[doi:10.31399/asm.hb.v23.a0005669.](https://doi.org/10.31399/asm.hb.v23.a0005669)

[31] T. DebRoy, H.L. Wei, J.S. Zuback, T. Mukherjee, J.W. Elmer, J.O. Milewski, A.M. Beese, A. Wilson-Heid, A. De, W. Zhang. "Additive manufacturing of metallic components – Process, structure and properties ". *Prog. Mater. Sci.* 92 (2018),pp: 112–224.

[doi:10.1016/j.pma-tsci.2017.10.001.](https://doi.org/10.1016/j.pma-tsci.2017.10.001)

[32] K.G. Prashanth, J. Eckert. " Formation of metastable cellular microstructures in selective laser melted alloys". *J. Alloys Compd.*(2017), Vol. 707 ,pp. 27–34.

[doi:10.1016/j.jallcom.2016.12.209.](https://doi.org/10.1016/j.jallcom.2016.12.209)

[33] [ASTM], "Standard test methods of tension testing of metallic materials ",American Association highway and transportation official standard (AASHTO) no.T88.