

2-23-2026

Synergistic Effect of Different Ions and Hexadecyltrimethylammonium Bromide on Wettability Alteration for Carbonate Rock

Rafal S. Abdullah

Department of Chemical Engineering, College of Engineering, University of Baghdad, Baghdad, Iraq,
rafal.abdullah2207m@coeng.uobaghdad.edu.iq

Hussein Q. Hussein

Department of Chemical Engineering, College of Engineering, University of Baghdad, Baghdad, Iraq,
husseinqassab@coeng.uobaghdad.edu.iq

Rana R. Jali

Research and Development Center, Ministry of Oil, Baghdad, Iraq, rana_rasool@prdc.oil.gov.iq

Follow this and additional works at: <https://bsj.uobaghdad.edu.iq/home>

How to Cite this Article

Abdullah, Rafal S.; Hussein, Hussein Q.; and Jali, Rana R. (2026) "Synergistic Effect of Different Ions and Hexadecyltrimethylammonium Bromide on Wettability Alteration for Carbonate Rock," *Baghdad Science Journal*: Vol. 23: Iss. 2, Article 1.

DOI: <https://doi.org/10.21123/2411-7986.5193>

This Article is brought to you for free and open access by Baghdad Science Journal. It has been accepted for inclusion in Baghdad Science Journal by an authorized editor of Baghdad Science Journal.



RESEARCH ARTICLE

Determination of Mebeverine – HCl Using 3, 5–Dinitrosalicylic Acid and Multiple Continuous Flow Cell That Works as a Solo Flow Cell with 4S×3 – 3D Analyzer

Elham N. Mezaal^{1,*}, Nagam S. Turkey²¹ Department of Chemistry, College of Education for Pure Sciences (Ibn-Al-Haitham), University of Baghdad, Baghdad, Iraq² Department of Chemistry, College of Science, University of Baghdad, Baghdad, Iraq**ABSTRACT**

A new method, simple and sensitive was utilized in determining mebeverine – HCl (MB-HCl) (3, 4-Dimethoxy benzoic acid ethyl 2, 4 methoxy4-phenyl-1-methyl ethyl amino-butyl ester) in pure and pharmaceutical formulations via utilization this multiple continuous flow cell. The method is dependent on genesis for complex of ion pair(4-((3, 4-dimethoxybenzoyl) oxy)-N-ethyl-N-(1-(4-methoxyphenyl) propan-2-yl) butan-1-aminium-2-hydroxy-3,5-dinitrobenzoate) among mebeverine–HCl (MB-HCl) and 3,5-Dinitrosalicylic acid (3,5-DNSA) in ammonium acetate middle to configure a whiteish yellow precipitate compound via utilizing multiple continuous flow cell that works as a solo flow cell with 4S×3 – 3D analyzer. Optimum parameters were studied to raise the sensitivity for improving the method. The linear dynamic range of calibration graph 0.5 – 60 mmol / L and LOD 582.5 ng /125 μL with correlation coefficient (r) 0.9783, RSD% was less than 0.5 %, (n = 6) for estimate of (MB-HCl) in concentration (13, 30) mmol / L. The results were compared together, traditional way method UV-Sp, via using the method of measuring additions by t-test and F-test, in 95% confidence plane. Comparing results explained that multiple continuous flow cell that works as a solo flow cell with 4S×3 – 3D analyzer is the good choice and widely utilized in applications.

Keywords: 3,5-Dinitrosalicylic acid, Flow injection analysis, Flow cell, Improved, Optimum parameters**Introduction**

Mebeverine–HCl (MB-HCl) is white crystalline, powder, molecular with weight = 466 g / mol, Molecular Formula = C₂₅H₃₅NO₅.HCl, Fig. 1. (MB-HCl) is soluble in water and ethanol, but not soluble in diethylether.¹ Mebeverine–HCl has name in IUPAC 3, 4-Dimethoxy benzoic acid ethyl 2, 4 methoxy4-phenyl-1-methyl ethyl amino-butyl ester. MB-HCl is widely utilized as a relaxant and antispasmodic medication of gastrointestinal tract especially colonic spasm and irritable bowel syndrome.²

Several analytical methods were revealed when scanning the literature to determine of mebeverine–HCl including simultaneous spectrophotometric method,³ ion association reaction,⁴ development method,⁵ pillarization technique⁶ HPLC,⁷ RP-HPLC,^{8,9} HPLC using degradation products,¹⁰ ion selective Electrodes,^{11,12} Voltammetry,^{13,14} potentiometric,¹⁵ and CFIA¹⁶ to estimate the pharmaceutical potion of MB-HCl. There are several other techniques that have been used to estimate some drugs, for example using HPLC,¹⁷ gas chromatography,¹⁸ RP-HPLC,¹⁹ CFIA,²⁰ and a new method was introduced within the continuous

Received 14 March 2024; revised 16 July 2024; accepted 18 July 2024.
Available online 23 February 2026

* Corresponding author.

E-mail addresses: elham.n.m@ihcoedu.uobaghdad.edu.iq (E. N. Mezaal), nagamturkey@yahoo.com (N. S. Turkey).

<https://doi.org/10.21123/2411-7986.5202>

2411-7986/© 2026 The Author(s). Published by College of Science for Women, University of Baghdad. This is an open-access article distributed under the terms of the Creative Commons Attribution 4.0 International License, which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

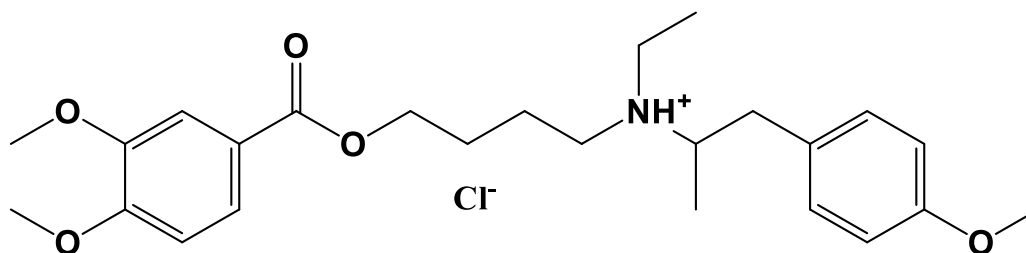


Fig. 1. Gestalt of Mebeverine–HCl (MB-HCl) (3, 4-Dimethoxy benzoic acid ethyl 2, 4 methoxy4-phenyl-1-methyl ethyl amino-butyl ester).

flow injection analysis technique using homemade cells which depend on fluorescence or turbidity as it is an easy, simple safe and inexpensive method to control the quality of DPH- cottoning drug tablets using homemade Ayah 6S \times 1-ST-2D.²¹ Therefore, we designed our experiment to improved FIA method, which is distinguished as easier, fast and very precise to measure the potion of MB-HCL within pharmaceutical formulations. Each drug has a different effect on the human body, so many researchers have resorted to study its effects, and we are one of those researchers.²²⁻²⁴ Other methods have been used by researchers to estimate using the uv-vis technique.²⁵

This research used multiple continuous flow injection analysis with turbidimetric measurement for MB-HCl determination using multiple continuous flow cell that works as a solo flow cell with 4S \times 3 – 3D analyzer. Measurements rely on (color whiteish yellow) the composition of the precipitated particles for MB-HCl - 3, 5-DNSA- CH₃COONH₄ system. Chemical factors were studied: concentration effect from reagent, effect of salt and acid medium of reaction and effect of ammonium acetate concentration as for the studied physical factors which include flow rate, volume sample and mixing coil. The best conditions studied were used to evaluate the drug and its application.

Materials and methods

All materials used are analytical reagents and dissolved by distilled water. The solution of standard 100 mmol/L of mebeverine-HCl was made via dissolving 4.6600 g in 100 ml of distilled water. A series of 3, 5-dinitrosalicylic acid solutions were made of the dilution for solution of standard 100 mmol / L together with water and be distilled.

Information about the apparatus


The request involved using triplet flow cell composed of three flow cells made of clear borax glass

in the form of tube, each of 60 mm length with inlet diameter of 2 mm, connected to these tubes a 600 mm Teflon tube into stages. Each of 300 mm length of 1mm was inside diameter. Intension in using two different diameter was used for different distances to insure good mixing and lengthen the flow cell in a total length of 3 \times 60 = 180 mm with 2mm inside diameter added to this length 600 mm of 1mm Teflon tube (hydrophobic). This 600 mm length was in the two stages, each of which is 300 mm. Two different materials were used : glass and Teflon, glass has a hydrophilic property via H- bonding with 2mm inside diameter i.e.; slow down fluid movement. On the contrary Teflon with 1mm inside diameter with its hydrophobic properties causes to enhance fluid movement i.e.; different fluid speed and delay or enhance movement causes much homogenization of fluid stream containing precipitated particulate and allowing enough time to give smooth noise – free responses as main homogeneity occur in the Teflon part which has no detection. Two stages recognized detection region and non-detecting location for completion of signal obtained in the glass tube and collect all these were in one single response of clean noise free response with excellent repeatability.²¹

Methodology

Using a manifold of two lines connected with 4S \times 3 – 3D analyzer to determine mebeverine-HCl via its reaction with 3, 5-dinitrosalicylic acid in ammonium acetate medium. It consists of 2 lines. One line as a vector current (CH₃COONH₄ 20 mmol / L) at 1.75 ml / min, the flow rate to for crossing during the valve of the injection to tote the segment from sample of mebeverine-HCl (20 mmol / L) run into one another 3, 5-dinitrosalicylic acid (5 mmol/L) in line two 1.75 ml/min of flux an average for reagent in Y-junction dot prior it is come into 4S \times 3 – 3D analyzer.²¹

Scheme 1 prospect mechanism for reaction of mebeverine-HCl together with 3, 5-dinitrosalicylic acid in ammonium acetate medium.

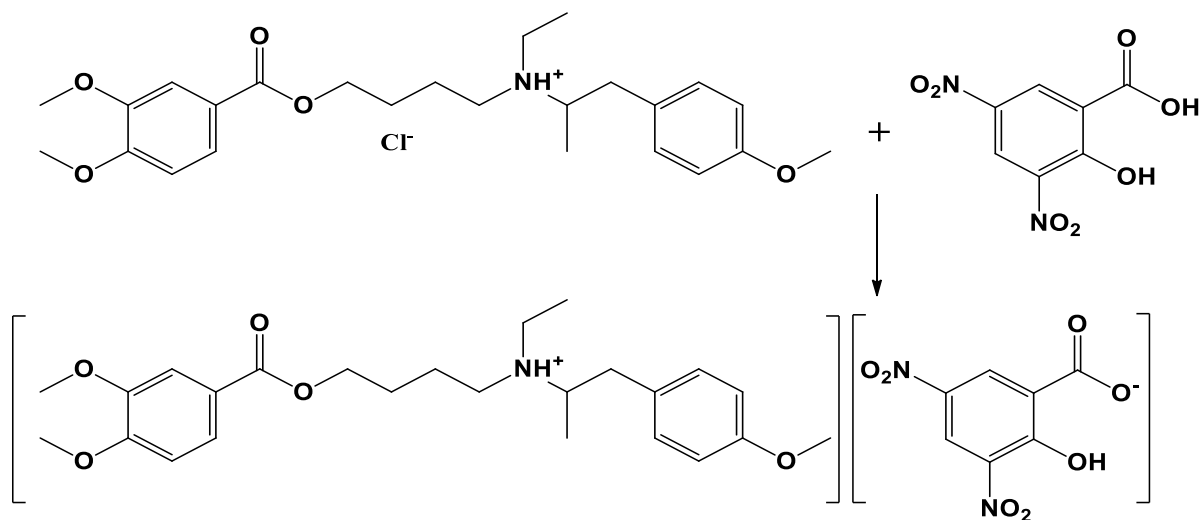

Scheme 1. Displays in prospect mechanism interaction path of mebeverine-HCl together with 3, 5-dinitrosalicylic acid in ammonium acetate medium.

Scheme 1. Displays in prospect mechanism interaction path of mebeverine-HCl together with 3, 5-dinitrosalicylic acid in ammonium acetate medium.

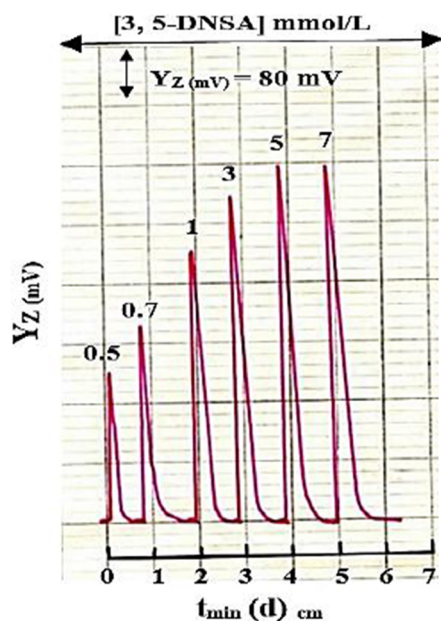


Fig. 2. Effect of variable concentration of 3, 5-Dinitrosalicylic acid (3, 5-DNSA) on: profile (S/N response to the power adapter).

Results and discussion

Optimization of variable

- Chemical variables

Concentration effect from reagent

A range of concentrations of 0.5–7 mmol/L of 3, 5-DNSA reagent was studied using a 125 μ L volume of sample injected through a conveyor stream. 20 mmol/L of MB-HCL was injected at a flow rate of

Table 1. Effect variable concentration from 3, 5-DNSA on the response of the transducer S/N for MB-HCL 20 mmol/L - 3, 5-DNSA system, utilization flow rate for each line 1.5 ml / min and 125 μ L of sample volume.

[3,5-DNSA] mmol/L	Average for peak heights (n = 3) $\bar{Y}_{Zi(mV)}$	$\bar{Y}_{Zi(mV)} \pm t$ SEM
0.5	253	253 \pm 1.23
0.7	334	334 \pm 1.56
1	455	455 \pm 1.98
3	542	542 \pm 2.24
5	595	595 \pm 2.98
7	590	590 \pm 2.31

Note. $\bar{Y}_{Zi(mV)}$: (S/N) response to the power adapter (i.e.; the average height of the peaks for n = 3 in mV. $t_{0.05/2, n-1} = t_{0.025, 2} = 4.303$, SEM = standard error of mean, t SEM = confidence interval.

1.5 mL/min per line. **Fig. 2** shows an increase in peak height with increasing concentration of 3, 5-DNSA. This is likely due to increasing the color of the deposited particles, which work to absorb part of the light. While at a concentration higher than > 5 mmol/L this may lead to increased agglomeration of particles and an increase in the spaces between those particles, which helps to penetrate a greater amount of light and reduce the height of the response. Therefore 5 mmol/L was chosen as the optimal concentration of 3, 5-DNSA reagent. The results obtained are shown in the **Table 1**.

Effect of salt and acid

The reaction between MB-HCL (20 mmol/L) with 3,5-DNSA (5 mmol/L) to form a whiteish yellow color precipitate was studied in various saline

Table 2. The effect of the difference in the middle on response measurement to the power adapter for determination MB-HCl.

Type for medium Salt (30 mmol/L) Acid (50 mmol/L)	Average for peak heights (n = 3) $\bar{Y}_{Zi(mV)}$	$\bar{Y}_{Zi(mV)} \pm t$ SEM at 95%
Water	595	595 ± 2.98
Sodium chloride	382	382 ± 3.13
Ammonium chloride	486	486 ± 2.97
Sodium acetate	302	302 ± 2.94
Ammonium acetate	644	644 ± 2.31
Potassium chloride	438	438 ± 3.42
Potassium nitrate	503	503 ± 2.49
Ascorbic acid	238	238 ± 1.92
Tartaric acid	331	331 ± 1.78
Salicylic acid	519	519 ± 3.22
Acetic acid	428	428 ± 2.32
Hydrochloric acid	489	489 ± 3.21

Note. $t_{0.05/2, n-1} = t_{0.025, 2} = 4.303$, SEM = standard error of mean, t SEM = confidence interval.

environments (sodium chloride, ammonium chloride, sodium acetate, ammonium acetate, potassium chloride, potassium nitrate) at 30 mmol / L and various acidic media (ascorbic acid, tartaric acid, salicylic acid, acetic acid, hydrochloric acid) at a concentration of 50 mmol / L in addition to the aqueous medium as a carrier current. The study showed that different media reduce the S/N response. This may be attributed to increasing the conglomeration and the intensity of fusion together and then raising the intensity of the light through it as there will be more empty spaces amidst the conglomerations of the particles except for the ammonium acetate which leads to an increase in the S/N response due to the effect of small solid particles which may lead to a reduction of the spatial areas and an increase in the limit from the incident light. Therefore ammonium acetate medium was used as vector current in the following studied. A results obtained are shown in Table 2.

Effect of ammonium acetate concentration

The reaction between MB-HCl (20 mmol/L) with 3,5-DNSA (5 mmol/L) to form a whiteish yellow color precipitate was studied at variable concentrations of ammonium acetate ranging (5–35 mmol/L) as a carrier stream in order to decide the most favorable concentration that will fit the methodology that was adopted in this conducted research work. It was noticed that a raise for ammonium acetate concentration up to 20 mmol/L leads to increased solubility or dissociation of some of the precipitate particles. Mostly the shape will be particles of small size can be mainly nucleus shaped which in turn will aid in clumping, leading to increased attenuation of incident light. More than 20 mmol/L leads to an increase of solubility of small size particulate. Therefore

Table 3. The effect for ammonium acetate concentration in the measurement of response to the power adapter for determination of MB-HCl using MB-HCl (20 mmol/L) - 3, 5-DNSA (5 mmol / L) system, 125 μ L the volume of sample in 1.5 ml/min flow rate of each line.

[Ammonium acetate] [CH ₃ COONH ₄] mmol/L	Average for peak heights (n = 3) $\bar{Y}_{Zi(mV)}$	$\bar{Y}_{Zi(mV)} \pm t$ SEM at 95%
5	452	452 ± 2.13
7	489	489 ± 2.91
10	502	502 ± 2.98
13	578	578 ± 3.12
15	620	620 ± 2.37
20	698	698 ± 3.21
25	666	666 ± 3.98
30	644	644 ± 2.31
35	560	560 ± 3.21

20 mmol/L of ammonium acetate concentration was chosen as optimum carrier stream. The set of results obtained are summarized in Table 3.

- Physical parameter

Flow rate

Using all previous experimental factors related to chemicals difference concentrations for complementary materials of this reaction of MB-HCl (20 mmol/L) - 3, 5-DNSA (5 mmol/L) - CH₃COONH₄ (20 mmol / L) system. Changing of flow rate was carried out utilizing 0.55–3.0 ml / min for each line. It was noticed that a raise in S/N- response profile up to 1.75 ml/min, the carrier current that might be attributed to the conglomerate has added a hardness to the particulate and it's weight on the other will cause compression and act as a wall because of its bigger size and bigger than the wavelength, so it will allow it to reflect all wavelengths and raise the attenuating of incident light. At rise speed more than 1.75 ml / min carrier stream might be to form a tiny or semi-transparent particulates and therefore, the light falling on it will suffer whatever its source is a reflection or refraction inside and outside the precipitating particulates causing a reduce to an insignificance level as shown by the obtained responses. Therefore; 1.75 ml/min of flow rate for each line. The results are summarized as in the Table 4.

The volume of sample

The effect for the volume of sample was studied utilizing using variable volume of teflon tube ranging (50–200) μ L of diameter (D) 1 mm.

High sample volume is not a recommended in the CFIA as a methodology as this type of scale will form

Table 4. Different effect for flow rate on the attenuation of incident light using 125 μL and 20 mmol/L concentration for MB-HCl and concentration 5 mmol/L for 3,5-DNSA.

Pump speed	flow rate (ml/min) for each Line1, Line2	Average for peak heights (n = 3) $\bar{Y}_{Zi(mV)}$	$\bar{Y}_{Zi(mV)} \pm t$ SEM at 95%	Base width Δt (sec)	V_{add} (m l) in flow cell	Concentration (mmol / L) in flow cell	Df in flow cell
5	0.55	588	588 \pm 3.15	70	1.4083	1.7752	11.27
10	0.75	593	593 \pm 3.12	45	1.2500	2.0000	10.00
15	1.25	620	620 \pm 2.97	35	1.5833	1.5790	12.67
20	1.5	698	698 \pm 3.21	28	1.5250	1.6393	12.20
25	1.75	753	753 \pm 2.42	25	1.5833	1.5790	12.67
30	2.00	750	750 \pm 2.23	22	1.5917	1.5706	12.73
35	2.25	701	701 \pm 2.13	21	1.7000	1.4706	13.60
40	2.50	688	688 \pm 1.98	20	1.7912	1.3957	14.33
45	3.00	610	610 \pm 1.38	19	2.0250	1.2346	16.20

Note. Δt : (sec) base breadth of peak, Df: dilution factor for a measured cell.

Table 5. The impact for difference volume for segment on reduction for incident light via concentration 20 mmol / L for MB-HCl together concentration 5 mmol/L for 3, 5-DNSA and a flow rate of the each line 1.75 ml/min.

Sample volume (μL)	Average for peak heights (n = 3) $\bar{Y}_{Zi(mV)}$	$\bar{Y}_{Zi(mV)} \pm t$ SEM at 95%	Base width Δt (sec)	V_{add} (ml) in flow cell	Concentration (mmol / L) in flow cell	Df in flow cell
50	400	400 \pm 1.35	18	1.1000	0.9091	22.00
75	510	510 \pm 1.67	20	1.2417	1.2080	16.56
100	633	633 \pm 2.34	22	1.3833	1.4458	13.83
125	753	753 \pm 2.42	25	1.5833	1.5790	12.67
150	745	745 \pm 2.97	27	1.7250	1.7391	11.50
175	740	740 \pm 2.48	29	1.8667	1.8750	10.67
180	710	710 \pm 3.12	30	1.9300	1.8653	10.72
200	700	700 \pm 3.97	31	2.0083	1.9917	10.04

locally in the concentration of a precipitate that can decompose, i.e.; at least part of it due to the continuous flow of carrier current which will result in K_{sp} of the precipitate > from doubling the concentration of the reactant species raising to the strength of their participation in the contributing force.

Low sample size will represent a rapid passage of the reaction product in front of the detector, which is solar cells that are not characterized by a fast response compared to PMT that can be detected at the nanosecond level. Therefore, a very small sample size may not be an appropriate choice, so the solution in this study was to choose an appropriate size 125 μL , and the results shown in the Table 5 were obtained.

Mixing coil

The effect of the reaction coil size on the peak height was studied, as it is attached before the measuring cell. Coil sizes from 0 to 350 μL were used. Whilst preservation all other changeable steady (MB-HCl (20 mmol / L), 3, 5-DNSA (5 mmol / L), the flow rate for each line (ammonium acetate and 3,5-DNSA) equal 1.75 ml / min, volume of sample 125 μL . The raise of volume coil leads to reduce and distort profile within raise of the base amplitude and departure time of the injected sample section via the

valve reaching into the cell. This may be attributed to the diffusion and dispersal that occur of precipitated particles for sample which in turn causes a raise of dispersed regions and especially lead to piling up for the precipitate particles, leading to an increase the inter-spaces between large precipitate particles that causes reduction in the attenuation of incident light. So its ability can be seen clearly at 100 μL the mixing coil necessary of completion the reaction among MB-HCl with 3, 5-DNSA in ammonium acetate ($\text{CH}_3\text{COONH}_4$) medium. Table 6. tabulates all the results.

Assessment of linear range for the scatter plot of difference for mebeverine- HCl against response S/N to the power adapter

A range of mebeverine – HCl concentrations (0.5–100 mmol/L) was used, and the peak height was measured with the best chemical and physical variables. The height of the transducer response increases when the sample concentration is increased. Fig. 3 explains the contrast ranges (the scatter of plot in the run (0.5–100) mmol / L, the dynamic range at (0.5–80) mmol / L, working range at (0.5–70) mmol / L and linear dynamic range at (0.5–60) mmol / L. The results summed up in the Table 7.

Table 6. Effect volume of reaction coil on energy transducer response expressed as an average peak heights (mV) for determination of MB-HCl (20 mmol / L) by 3,5-DNSA (5 mmol / L), 1.75 ml / min flow rate for vector current and 125 μ L volume of sample.

Volume of reaction coil (μ L)	Average for peak heights (n = 3) $\bar{Y}_{Zi(mV)}$	$\bar{Y}_{Zi(mV)} \pm t$ SEM at 95%	Base width Δt (sec)	V_{add} (ml) in flow cell	Con. (mmol / L) in flow cell	Df in flow cell
0*	753	753 \pm 2.42	25	1.5833	1.5790	12.67
100	788	788 \pm 2.42	28	1.7583	1.4218	14.07
200	760	760 \pm 3.21	35	2.1667	1.1538	17.33
250	632	632 \pm 3.49	40	2.4583	1.0170	19.67
300	600	600 \pm 4.21	46	2.8083	0.8902	22.47
350	588	588 \pm 4.32	52	3.1583	0.7916	25.27

Note. 0* without coil, Δt : sec breath of peak.

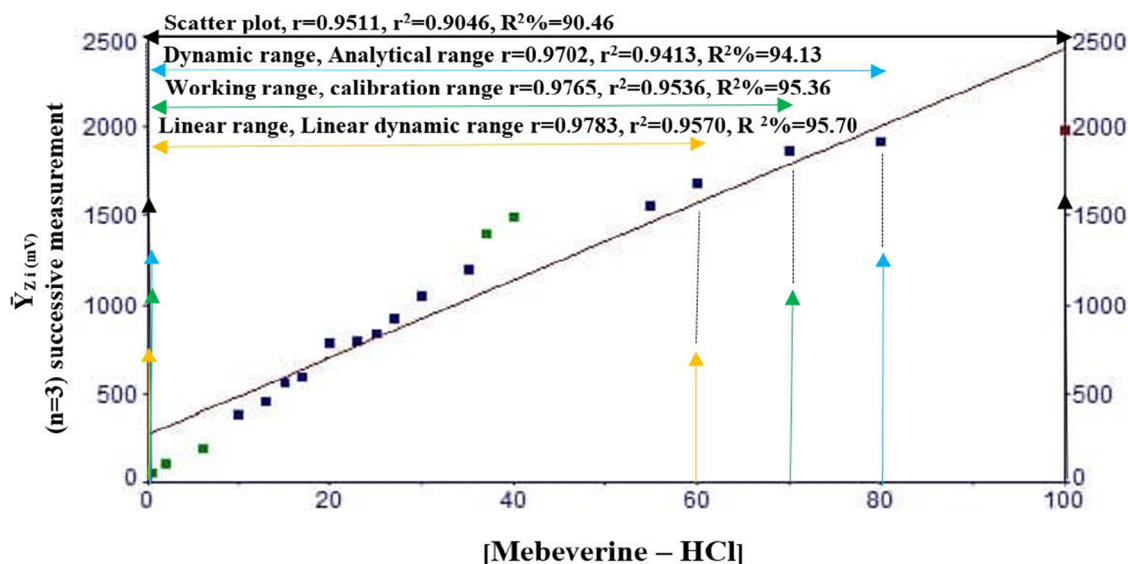


Fig. 3. Effect for Variable range of concentration of mebeverine – HCl on reduction of incident light, scatter plot in range (0.5–100) mmol / L for n = 20, dynamic range at (0.5–80) mmol / L for n = 19, working range at (0.5–70) mmol / L for n = 18 and linear range at (0.5–60) mmol / L for n = 17.

Table 7. The result of linear regression for difference of response S/N to the power adapter together with concentration of mebeverine – HCl using the equation for the first degree as in the model $\hat{Y} = a + bx$ in the best conditions.

Mode species	[MB-HCl] extent mmol / L(n)	$\hat{Y}_{Zi(mV)} = a_{mV} \pm S_a t + b (\Delta y_{mV} / \Delta x_{mmol/L}) \pm S_b t$ [MB-HCl] mmol / L in confidence level 95%, n-2	r, r ² , R ² %	t _{tab} at 95%, n-2	Calculated t-value t _{cal} = r / $\sqrt{n-2} / \sqrt{1-r^2}$
Scatter plot	0.5–100 (20)	273.8208 \pm 147.6076 + 21.5922 \pm 3.4732 [MB-HCl] mmol/L	0.9511, 0.9046, 90.46	2.101	<< 13.0644
Dynamic range or analytical range	0.5–80 (19)	195.7670 \pm 118.5436 + 25.0160 \pm 3.1969 [MB-HCl] mmol/L	0.9702, 0.9413, 94.13	2.110	<< 16.5107
Working range or calibration range	0.5–70 (18)	149.7945 \pm 105.7325 + 27.3114 \pm 3.1940 [MB-HCl] mmol/L	0.9765, 0.9536, 95.36	2.120	<< 18.1331
Linear range or linear dynamic range	0.5–60 (17)	113.5844 \pm 100.7933 + 29.2781 \pm 3.4132 [MB-HCl] mmol/L	0.9783, 0.9570, 95.70	2.131	<< 18.2719

Note. n: number of measurement, $\hat{Y}_{Zi(mV)}$: evaluated value in mV for improved method, r: correlation coefficient for each range, r²: coefficient for estimation, R²% = percentage capital R-squared: explained difference as a percentage / total difference and t_{tab} = t_{0.05 / 2, n-2}.

Table 8. Limit of detection of mebeverine – HCl at best parameters using 125 μL as an injection from sample volume, 1.75 ml / min flow rate for both line, 3, 5-DNSA (5 mmol / L).

Practically based on the progressive mitigation of lower concentration in scatter plot (0.5 mmol / L)	Theoretical based on the amount of slope $x = 3 S_B / \text{slope}$	Theoretical based on of the linear equation $\hat{Y} = Y_b + 3S_b$
0.01 mmol/L 582.5000 ng / 125 μL	1.7883 μg / 125 μL	653.2839 μg / 125 μL

Note. X = LOD based on slope from linear dynamic range and S_B = standard deviation of blank refined for 13 times Y_b = rate response of blank= an intercept, S_b = standard deviation amounting into S_y / x = residual from linear dynamic range, \hat{Y} : estimated response (mV).

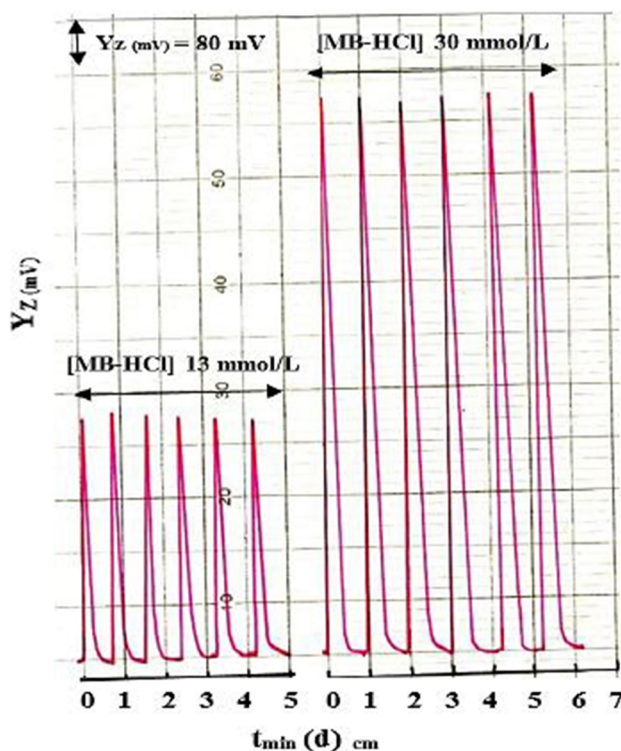


Fig. 4. Response to six successive repeatable measurement concentration of mebeverine – HCl (13 and 30 mmol / L) using 3, 5-DNSA (5 mmol / L), 1.75 ml / min flow rate for each line and 125 μ L volume of sample.

Table 9. Repeatability of mebeverine – HCl in best parameters with 125 μ L volume of sample.

[MB – HCl] (mmol / L)	Average for peak heights (n = 6) \bar{Y}_{Zi} (m V)	RSD %	Confidence interval in (95%) $\bar{Y}_{Zi(mV)} \pm t_{0.05/2, n-1} \sigma_{n-1} / \sqrt{n}$
13	460	0.1304	460 ± 0.6298
30	1050	0.1247	1050 ± 1.3750

Note. (n= 6) the number of injections, $t_{tab} = t_{0.05/2,7} = 2.365$.

LOD

Limit of detection (LOD) was studied for mebeverine – HCl during three different approach as shown in the Table 8. as an injected 125 μ L from sample volume.

Repeatability

The relative standard deviation = RSD % of mebeverine – HCl for 13 and 30 mmol / L as shown in

Table 9. The relative standard deviation minimal than 0.5 % was obtained indicating that via using this method, a reliable measurement can be achieved using this way. Fig. 4 shows the response profile.

Assessment of multiple continuous flow cell that works as a solo flow cell with 4S×3 – 3D analyzer for determination of mebeverine- HCl in drugs

The newly developed methodology mebeverine – HCl was estimated in three drugs from three

Table 10. Standard addition method for determination of MB – HCl in three types of drugs utilization multiple continuous flow cell that works as a solo flow cell with 4S×3 – 3D analyzer and classical method UV- Spectrophotometric (UV-Sp.).

		Type of method										
		Newly developed methodology										
		UV- Spectrophotometric (UV-Sp.) traditional method absorbance measure in $\lambda_{max} = 219 \text{ nm}$										
No. for sample	Commercial name, Country, Content	Confidence interval for the rate Weight of tablet $\bar{w}_1 \pm 1.96 \sigma_{n-1} / \sqrt{n}$ in 95 % g	Theoretical content of the active ingredient in 95 % (mg) $\bar{w}_1 \pm 1.96 \sigma_{n-1} / \sqrt{n}$	Practical of concentration (mmol / L) in 100 ml in	Efficiency of determination Rec.% Newly method (UV-Sp.)	t-test the comparison among methods		F-test the comparison among methods		r	r^2	$R^{2\%}$
						$t_{cal} = \frac{\bar{X}d}{\sigma_{n-1} \sqrt{n}}$	t_{tab} in 95% confidence level	$F_{cal} = \frac{S^2_1}{S^2_2 (UV-Sp.)}$	F_{tab}			
1	Duspatalin, Abbott, France, 135 mg	0.4183 ± 0.0028	135 ± 0.9036	2.0850	104.25	$\bar{X}d = -3.8461$	t_{tab} in 95% confidence level	$F_{cal} = \frac{S^2_1}{S^2_2 (UV-Sp.)}$	F_{tab}	0.9866	0.9734	97.34
2	Meva, Jamjoom Pharma, Saudi Arabia, 135 mg	0.4035 ± 0.0021	135 ± 0.7026	5.2134	104.35	$\sigma_{n-1} = 5.4662$	$-1.2187 / < 4.303$	$\sigma^*_{n-1} = 3.9048$, $S^2_1 = 15.2475$	$F_{cal} = \frac{S^2_1}{S^2_2 (UV-Sp.)}$	0.9981	0.9962	99.62
3	Colospasmin, Eipico, Egypt, 135 mg	0.3621 ± 0.0034	135 ± 1.2676	1.9730	98.67			$\sigma^*_{n-1} = 1.7073$, $S^2_2 = 2.9149$	$F_{cal} = \frac{S^2_1}{S^2_2 (UV-Sp.)}$	0.99974	0.99949	99.949

Note. $\bar{X}d$: the average of variation between two method (improved & traditional), n(number for sample) = 3, σ_{n-1} : standard of deviation for variation, \bar{W}_i : mg practically weight, $t_{tab} = t_{0.05/2,2} = 4.303$ of t-test, $F_{tab} = F_{0.95, V1, V2} = F_{0.95, 2, 2} = 39$, σ^*_{n-1} : standard deviation (F-test), UV-Sp. : UV- Spectrophotometric, S^2_1 = variation for developed method, S^2_2 = variation of classical method (UV- Spectrophotometric), $t_{tab} = t_{0.05 / 2, \infty} = 1.96$ at 95%.

Table 11. Result obtained by other researchers.

Method	Reagent	Linear rang	RSD%	R	Ref.
Potentiometric	Poly vinyl chloride	$1 \times 10^{-1} - 1 \times 10^{-6}$ M	< 2%	1.0000	¹²
Turbidmetric	Sodium persulfate	2–10 $\mu\text{mol.L}^{-1}$	< 1%	0.9981	¹⁶
Multiple continuous flow cell	3,5-dinitrosalicylic acid	0.5–60 mmol.L^{-1}	< 0.5%	0.9783	-

different companies Duspatalin, Abbott, France, 135 mg, Meva Jamjoom, Pharma, Saudi Arabia, 135 mg and Colospasmin, Eipico, Egypt, 135 mg.

A multiple continuous flow cell that works as a solo flow cell with 4S×3 – 3D analyzer for the determination of mebeverine – HCl in drugs and was compared with method which includes UV-Spectrophotometric. A several of sol were intended for each drug (5 mmol / L) by transferring 4 ml to each of five volumetric flask (10 m L) he follows by the addendum of 0, 0.2, 0.4, 0.6 and 0.8 ml from 50 mmol / L for standard solution of drug to get 0, 1, 2, 3 and 4 mmol / L for suggested method. The results were processed mathematically using the method of measurement additions. Table 10 shows practical content of active ingredient in 95% confidence plane and efficiency for the appreciation in addendum to the t-test and F-test. The obtained results no significant variation amidst improved and traditional method in 95% the plane of confidence for estimation of mebeverine – HCl in pharmaceutical drugs.

Table 11 showing a comparison of the results obtained by other researchers in estimating the same drug and using different methods.

Conclusion

The assessment of multiple continuous flow cell that works as a solo flow cell with 4S×3 – 3D analyzer among this research action was applied using comparison among 4S×3 – 3D analyzer with classical UV-spectrophotometric method using mebeverine–HCl (MB-HCl) with 3,5-Dinitrosalicylic acid in medium ammonium acetate. In this research work the physical and chemical factors were studied. It was known that a narrower extent is obtained together UV-spectrophotometric kind, whilst widely extent was property for 4S×3 – 3D analyzer. A multiple continuous flow cell that works as a solo flow cell with 4S×3 – 3D analyzer is the option together with excellent detection range and a wide application. Future use a multiple continuous flow cell that works as a solo flow cell with 4S×3 – 3D analyzer for estimation and study most of the drugs that are chosen.

Acknowledgment

Author express their sincere thanks and appreciation to Prof. Dr. Issam Mohamed Ali Shakir for offering valuable devices for completing the research.

Authors' declaration

- Conflicts of Interest: None.
- We hereby confirm all the Figures and Tables in the manuscript are ours. Any Figures and images, that are not ours, have been included with the necessary permission for re-publication, which is attached to the manuscript.
- No animal studies are present in the manuscript.
- Author(s) signed on ethical consideration's approval.
- Ethical Clearance: The project was approved by the local ethical committee at University of Baghdad.

Authors' contribution statement

N.S.T. conceived of the presented idea, E.N.M. performed the computations and wrote the manuscript.

References

1. Ahmed HN, Ahmed K, Ahmed AG, Mahmoud HM, Abd El-Aziz YE, Adel AA. Graphite studded with facile-synthesized Cu₂O nanoparticle-based cubes as a novel electrochemical sensor for highly sensitive voltametric determination of mebeverine hydrochloride. *Chemosensors*. 2021;9(35):1–22. <https://doi.org/10.3390/chemosensors9020035>.
2. Parag M, Senthilkumar GP. Development and validation of HPLC method for determination of degradation impurities for the qualification of Mebeverine HCL. *Am J Pharm Tech Res*. 2020;10(1):137–147. <https://doi.org/10.46624/ajptr.2020.v10.i1.012>.
3. Hayam ML, Yasmin MF, Adel MM, Christine KN. Simultaneous determination of mebeverine hydrochloride and chlordiazepoxide in their binary mixture using novel univariate spectrophotometric methods via different manipulation pathways. *Spectrochimica Acta Part A: Spectrochim Acta A Mol Biomol Spectrosc*. 2016;155(15):11–20. <https://doi.org/10.1016/j.saa.2015.10.033>.

- Abdulbari M, Zainab A. Spectrofluorimetric determination of mebeverine hydrochloride in pharmaceutical preparation via ion association reaction. *J Phys Conf Ser.* 2018;1032:1–9. <https://doi.org/10.1088/1742-6596/1032/1/012064>.
- Pallavi A, Balakrishnaiah P, Srinivasa RY, Vara PR, Vasudha D. New uv- spectrophotometric method development and validation of mebeverine HCL in pure and formulation. *I J B P A S.* 2022;11(7):3029–3036. <https://doi.org/10.31032/IJBPAS/2022/11.7.6203>.
- Parchaki P, Sunitha R. Formulation and evaluation of mebeverine hydrochloride sustained release capsules by pelletization technique. *Saudi J Med Pharm Sci.* 2022;8(11):644–649. <https://doi.org/10.36348/sjimps.2022.v08i11.002>.
- Parag M, Senthilkumar GP. Development and validation of HPLC method for determination of degradation impurities for the qualification of mebeverine HCL. *Am J Pharm Tech Res.* 2020;10(1):137–147. <https://doi.org/10.46624/ajptr.2020.v10.i1.012>.
- Puvvada VK, Karavadi T, Saibabu Ch. Method development and validation of mebeverine hydrochloride in capsules by RP-HPLC. *Int J Res Publ Rev.* 2023;4(7):2814–2825. <https://doi.org/10.47119/27083578>.
- Marella VL, Pavani M, Garikapati DR. RP-HPLC method for determination of mebeverine Hydrochloride in dosage forms employing ms compatible buffers. *IDMA.* 2020;57(3):69–72. <https://doi.org/10.53879/id.57.03.11722>.
- Rania NE, Fathalla FB. Simultaneous HPLC determination of chlordiazepoxide and mebeverine HCL in the presence of their degradation products and impurities. *J Chem.* 2015;1–9. <https://doi.org/10.1155/2015/293719>.
- Tamer AA, Gehad GM, Omar MM, Veronia NA. Improved determination of mebeverine hydrochloride in urine, serum and pharmaceutical preparations utilizing a modified carbon paste electrode. *Int J Electrochem Sci.* 2015;10(3):2439–2454. [https://doi.org/10.1016/S1452-3981\(23\)04859-9](https://doi.org/10.1016/S1452-3981(23)04859-9).
- Inas HA, Yehya KA, Inas HA. A sensitive electrochemical sensor for rapid determination of mebeverine hydrochloride and metronidazole benzoate selective molecular imprinted polymer in the PVC membrane. *Ibn al-Haitham J Pure Appl Sci.* 2018;31(1):75–87. <https://doi.org/1030526/31.1.1855>.
- Azizollah N, Golnar AB. Multivariate optimization of mebeverine analysis using molecularly imprinted polymer electrochemical sensor based on silver nanoparticles. *J Food Drug Anal.* 2019;27:305–314. <https://doi.org/10.1016/j.jfda.2018.05.002>.
- Fared ME, Hanaa SE, Mohamed MG. A green method for the determination of mebeverine in its pharmaceutical products and human serum based on diatom modified carbon paste electrode using square wave adsorptive anodic stripping voltammetry (SW-AdASV). *Int Con Chem Envi Eng.* 2018;9(6):2–20. <https://doi.org/10.21608/iccee.2018.34645>.
- Ahmed MAR, Manal MF, Noha SR, Ahmed E, Ashraf A. Potentiometric determination of mebeverine hydrochloride antispasmodic drug based on molecular docking with different ionophores host–guest inclusion as a theoretical study. *RSC Adv.* 2023;13(2):1085–1093. <https://doi.org/10.1039/d2ra06127a>.
- Nagham T, Jalal NJ. Turbidimetric determination of mebeverine hydrochloride in pharmaceutical formulations using two consecutive detection zones under continuous flow conditions. *Chem Chem Technol.* 2022;16(4):600–613. <https://doi.org/10.23939/chcht16.04.600>.
- Zeinab A, Marwa S, Ekram HM, Fatma AF. Assessment of the greenness of micellar HPLC method for rapid separation and simultaneous estimation of chlorpheniramine maleate in presence of some co-administered drugs in three pharmaceutical dosage forms using single run. *Acta Chromatogr.* 2021;34(2):138–149. <https://doi.org/10.1556/1326.2021.00883>.
- Vishwas TS, Gurupadaya BM, Jain R. Stability indicating green analytical gas chromatography method for the determination of diphenhydramine in pure and marketed formulations. *Int J Pharm Sci Res.* 2019;10(9):4280–4286. [https://doi.org/10.13040/IJPSR.0975-8232.10\(9\).4280-86](https://doi.org/10.13040/IJPSR.0975-8232.10(9).4280-86).
- Viviane A, Teuku Nanda SS, Akhmad KN, Agung EN. Validation of RP-HPLC method for determination of pH-dependent solubility of ketoconazole in phosphate buffer pH 6.8. *J Res Pharm.* 2022;26(6):1694–1702. <https://doi.org/10.29228/jrp.260>.
- Turkey NS, Mezaal EN. Continuous flow injection analysis, turbidimetric and photometric determination of methyl dopa using a new long distance chasing photometer (NAG-ADF-300-2). *Indian J. Forensic Med. Toxicol.* 2020;14(4):1835–1841. <https://doi.org/10.37506/ijfmt.v14i4.11810>.
- Muntadhar MJ, Elham NM. Continuous flow injection analysis method for the determination of a drug diphenhydramine hydrochloride by using phosphomolybdic acid. *Baghdad Sci. J.* 2024;21(8). <https://doi.org/10.21123/bsj.2024.8926>.
- Camil CM, Roxana II, Dragos TI. Delta-radiomics entropy based on tumor heterogeneity concept – response predictor to irradiation for unresectable/recurrent glioblastoma. *Medic Mod.* 2022;29(4):273–278. <https://doi.org/10.31689/rmm.2022.29.4.273>.
- Camil CM, Roxana II, Mihai CS, Dragos PT, Florinel B. Cetuximab-taxanes-platinum-fluorouracil/capecitabine (C-TPF/C-TPX) – a feasible option for recurrent HNSCC with negative prognostic factors. Literature review with a case presentation. *Med Mod.* 2023;30(1):23–28. <https://doi.org/10.31689/rmm.2023.30.1.23>.
- Camil CM, Mihai CS, Roxana II, Dragos PT, Florinel B. Skin cancers of the head and neck region: the real world epidemiological and therapeutic data from the cancer registry of Dolj County. *Med Mod* 2023;30(3):175–180. <https://doi.org/10.31689/rmm.2023.30.3.175>.
- Mezaal E, Sadiq K, Rumez R. Spectrophotometric method for determination of Cu (II) using a new schiff base ligand. *J Appl Spectrosc.* 2024;91(1):236–245. <https://doi.org/10.1007/s10812-024-01711-1>.

تقدير الموبيفرين – حامض الهيدروكلوريك باستخدام حامض 5,3 – ثنائي نايتروسالسيك و خلية التدفق المستمر المتعددة التي تعمل كخلية تدفق منفردة مع محلل 4S× 3-3D

الهام نعيمش مزعل¹، نغم شاكر تركي²

¹ قسم الكيمياء، كلية التربية للعلوم الصرفة ابن الهيثم، جامعة بغداد، بغداد، العراق.

² قسم الكيمياء، كلية العلوم، جامعة بغداد، بغداد، العراق.

الخلاصة

تم استخدام طريقة جديدة وبسيطة وحساسة لتقدير عقار الموبيفرين في صورته النقية وفي المستحضرات الصيدلانية عن طريق استخدام خلية التدفق المستمر المتعددة. تعتمد الطريقة على تكوين معقد ايوني بين الموبيفرين والكاشف حامض 5,3-ثنائي نايتروسالسيك في وسط من خلاص الامونيوم لتكوين مركب راسب اصفر مبيض باستخدام محلل خلية التدفق المستمر المتعددة تعمل كخلية تدفق منفردة مع محلل 4S×3-3D. تمت دراسة الظروف المثلى لرفع الحساسية للطريقة المطورة. النطاق الديناميكي الخطي للمعايرة 0.5-60 مليمول / لتر وحدود كشف 582.5 نانو غرام لكل 125 ميكرو لتر مع معامل ارتباط 0.9783 وكان الانحراف القياسي النسبي المئوي اقل من 5% لعدد قراءات يساوي 6 لتقدير عقار الموبيفرين بتركيز 30,13 مليمول / لتر. النتائج تمت مقارنتها مع الطريقة التقليدية UV-Sp. وذلك باستخدام طريق اضافات القياس باستخدام اختبار t-test و اختبار F-test عند مستوى الثقة 95%. توضح نتائج المقارنة ان خلية التدفق المستمر المتعددة التي تعمل كخلية تدفق منفرد مع محلل 4S×3-3D هي الخيار الجيد وتستخدم على نطاق واسع في التطبيق.

الكلمات المفتاحية: حامض 5,3-ثنائي نايتروسالسيك، التحليل بالحقن الجرياني، خلية الجريان، تحسين، الظروف المثلى.